



Site 18-105-0003: , IN

Thermo Scientific Model 5030 SHARP w/VSCC

Continuous (y) vs. FRM (x) $PM_{2.5}$ ($\mu g \cdot m^{-3}$)

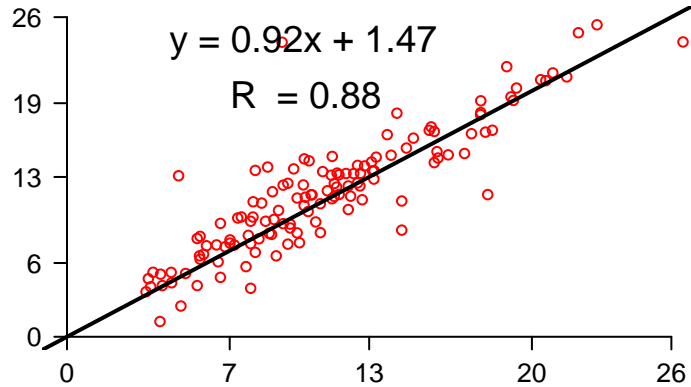


FRM minus Continuous $PM_{2.5}$ ($\mu g \cdot m^{-3}$)

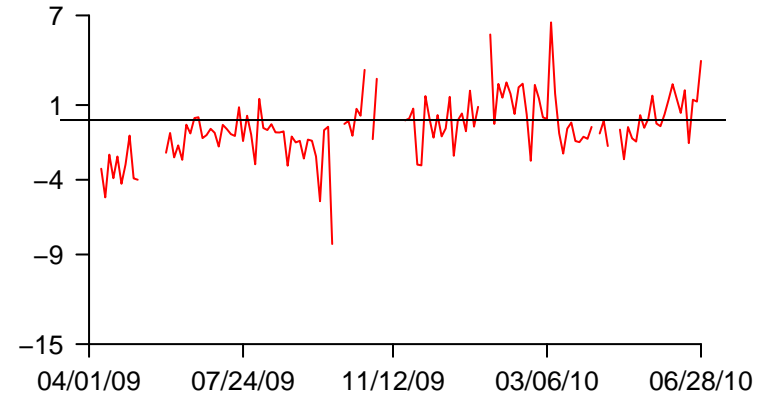


Mean $PM_{2.5}$ ($\mu g \cdot m^{-3}$)

	#	FRM	Con.	Ratio (Con/FRM)
○	130	11.2	11.8	1.05
▽	28	13.1	12.1	0.92
△	21	9.8	10.3	1.05
△	34	11.7	12.5	1.07
▽	47	10.3	11.7	1.14
9	75	11	12.4	1.13
0	55	11.4	11	0.96

Additive (y) vs. Multiplicative (x) Bias

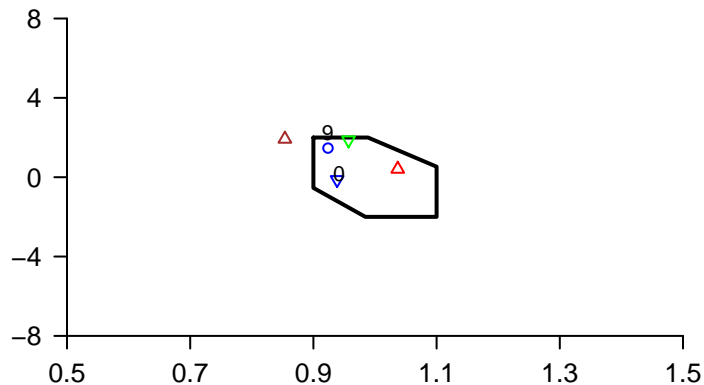

R (y) vs. FRM CCV (x)

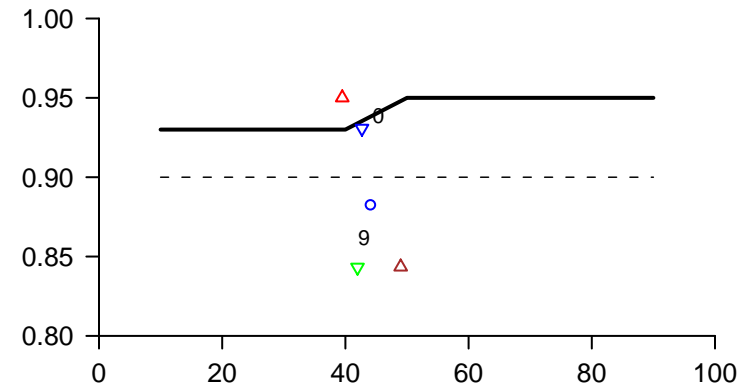

○ AllData △ Autumn ▽ Spring △ Summer ▽ Winter
8 2008 9 2009 0 2010